

A Wearable Pad for Detecting and Monitoring Heel Pressure Ulcer: Preliminary Study

S. Morad¹, A. M. Biju¹, and A. H. Morad²

¹ University of East London, London, UK

² Gilgamesh University, Baghdad, Iraq

Email: s.morad@uel.ac.uk (S.M.); u2228958@uel.ac.uk (A.M.B.); ameer.h.morad@gu.edu.iq (A.H.M.).

Manuscript received October 20, 2024; accepted December 7, 2024; published April 25, 2025.

Abstract—This paper addresses a critical gap in wearable sensors for pressure ulcer monitoring, focusing on heel pressure ulcer, a high-risk area. In This study, a wearable pad for monitoring pressure ulcers on bedridden patients was developed. The pad integrates pressure and temperature sensors into a comfortable fabric bandage, allowing for data collection and analysis. Machine algorithms classify sensor readings as healthy or risky, with a user-friendly display communicating the risk level. The wearable pad is tested on three individuals, recording the difference between a heel without pressure ulcer and one with an existing pressure ulcer. The successful development and validation of this wearable sensor pad could revolutionize early detection and prevention strategies for bedridden patients, improving health outcomes and reducing healthcare costs.

Keywords—pressure ulcer, wearable pad, monitoring sensors, machine learning

I. INTRODUCTION

Decubitus ulcers, also known as Pressure Ulcers (PUs), are a significant complication for bedridden patients, causing immense discomfort and serious health problems. Current preventative measures have limitations, particularly in monitoring heel PUs, which are anatomically complex and cannot be effectively offloaded by immobilization in a patient's bed. Shear force cannot be detected by current methods of PU measurement, leading to wound deterioration [1]. Heel PUs can last for months or years, prolonging hospital stays and increasing healthcare costs [2]. The lack of early detection between high and low risk ulcers causes them to progress into worse stages, characterized by tissue necrosis extending to the muscle and bone, causing severe pain and direct patient morbidity [3, 4].

These challenges highlight the need for heel-specific PU monitoring technology, specifically designed for early detection in the heel, a high-risk area for bedridden patients. This study aims to address the limitations of current prevention measures and improve early detection and prevention strategies for PUs in the heel region.

A. Overview of the Formation of Heel PUs

Heel pressure injuries occur when mechanical forces compress and deform tissues between the bony prominence of the calcaneus and the external surface [5, 6].

The posterior portion of the heel, which contains the inflexible Achilles tendon, has a low subcutaneous fat volume, making it vulnerable to pressure and tissue disintegration [7–9]. The heel is made up of skin covering the reticular dermis and avascular fat contained in fibrous septa compartments supplied by blood vessels [8]. The sole muscle in the heel is the thin layer of panniculus carnosus

muscle, which is likely responsible for forming heel pressure injuries (PU) [7, 8]. Heel PU may appear as dark, dry eschar areas or rankles packed with fluids or blood that eventually re-epithelialize behind the eschar [10]. The degree of tension applied is not often reflected in the severity of a heel pressure injury [7]. Early detection of tissue damage using skin staining may lead to more potent anticipation training and less severe skin damage. Subepidermal Moisture (SEM) is a biophysical measurement used to represent oedema in tissues below the layer corneum to distinguish it from moisture on the outer layer of the epidermis [11]. Heel pressure injuries are most common in bedridden people, as persistent pressure from lying flat for prolonged periods compresses blood vessels, limiting blood flow to the tissue, leading to ulcer development and cell death. Preventive measures can improve early detection and prevention strategies [5].

Fig. 1 shows a real-life image of heel PU for one of the subjects participated in this study. Evidently, the person's heel has soreness and is on the initial stage of PU.



Fig. 1. Heels of bedridden patient participated in this study with initial stage of PU.

B. Pressure Injuries

Pressure on the skin can cause physical and psychological responses, such as sensations like touch, pressure, and pain, and impact temperature regulation. However, excessive pressure can impede blood circulation, leading to conditions like PUs. PUs are characterized by localized skin and tissue damage due to factors such as pressure, friction, and internal health issues like malnutrition or anemia [12, 13].

The severity of PUs is assessed using systems like the National PU Advisory Panel (NPUAP) staging, which categorizes injuries into four stages based on tissue involvement. PUs often occurs over bony areas but can develop in various regions subjected to prolonged pressure. Multiple risk factors contribute to PU development, particularly in hospitalized patients with neurological or

cardiovascular diseases. Treatment involves pressure reduction, wound care, surgical intervention, and nutrition. Prevention strategies include regular patient repositioning, although the optimal interval remains uncertain [14]. Despite preventive efforts, the global incidence of PUs in hospitals remains around 12%, emphasizing the need for further research into their management and prevention [15].

C. Existing Methods for Heel PU Detection

- (1) Visual Inspection: Caretakers should regularly inspect heels for signs of skin redness or discoloration, which could indicate the formation of a PU [16]. However, darker skin tones may miss early signs, and routine visual inspections may not be sufficient at night to identify PUs in their early stages [17].
- (2) Palpation: Carers may palpate the heels to detect changes in skin temperature, stiffness, or soreness, which may indicate underlying tissue damage [18].
- (3) The redness/blanching test: involves applying pressure to the heel and measuring the time it takes for redness to return (Fig. 2), which can help determine blood flow rate [16].



Fig. 2. Skin blanching test done by nurses in patients using a clear plastic key fob to test a red area for blanching.

- (4) Pressure mapping systems: use pressure sensors to measure pressure distribution across the body, including the heels (Fig. 3). Although they don't directly assess blood flow or tissue damage, they provide valuable information but may miss early signs of tissue damage before skin changes appear [17].

D. Pressure-skin Temperature Relationship

Our bodies function like thermostats, regulating skin temperature through blood vessel opening and closing. Sweating helps maintain coolness. Air and wind temperature can also affect skin temperature, which can indicate medical conditions like fever or circulation issues. Variations in skin temperature can indicate these conditions.

This study uses infrared thermometers to measure skin temperature, which is categorized into contact methods like thermometry and non-contact methods like infrared thermometers [19]. Human body temperature is not constant, with greater variation in muscles and organs and lower in bone parts. The typical range for torso skin temperature is 33.5°C to 36.9°C, with infrared thermometers being used in this study [20]. Several studies have investigated the relationship between pressure and skin temperature, employing various methods such as pressure loading simulations and thermal imaging. For instance, research by Yoshimura *et al.* (2015) and Sae-Sia *et al.* (2005)

demonstrated a positive correlation between prolonged pressure loading and increased skin temperature in specific areas [21–22]. However, Mayrovitz *et al.* (2018) found no significant difference in skin temperature between high-risk and low-risk areas using thermal imaging [23]. Similarly, Sun *et al.* (2008) observed that high skin temperature wounds tended to progress to deeper damage compared to low-temperature wounds [24]. Continuous skin temperature measurements have also been utilized by Rapp *et al.* (2009) revealing lower entropy levels in patients who developed pressure ulcers, indicating reduced adaptability to stress [25]. Despite these findings, the debate continues regarding the association between skin temperature and PU development.

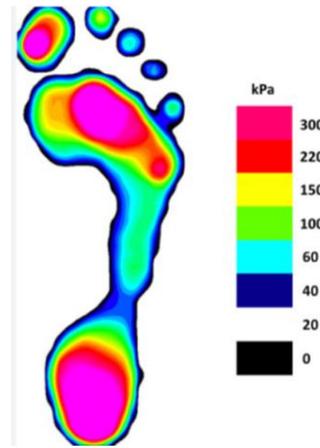


Fig. 3. Image of pressure mapping showing pressure distribution [17].

Two studies used a time series approach to analyze entropy, revealing potential indicators of PU risk. However, most used controlled pressure loading simulations or artificial stimuli, limiting generalizability. This study uses continuous measurements in a natural hospital setting to extract pressure events from time series data. This approach aims to provide insights into the complex relationship between pressure and skin temperature, improving risk assessment and prevention strategies for PU development.

E. Previous Work Done Relevant to This Study

Previous studies on PU (decubitus ulcers) have shown that early detection is crucial for preventing their progression. This review reviews existing research on wearable sensors for PU detection, focusing on heels, a high-risk area. Kim *et al.* [26] developed a fabric-based multifunctional sensor integrating pressure, temperature, and skin impedance sensors, showing promise for early detection. Other studies have explored various sensor types for PU detection, such as capacitive pressure sensors [27] and temperature sensors [18]. However, these studies do not address the specific challenges of heel PUs. Overall, the potential of different sensor modalities for PU detection remains unexplored.

II. MATERIALS AND METHODS

The PU in heels occur due to prolonged restriction of blood vessels to the underlying skin and tissues. Pressure monitoring is crucial as excessive pressure can lead to compression of blood vessels, resulting in cell death and ulcer formation [28]. Studies show a correlation between the

tool for early diagnosis.

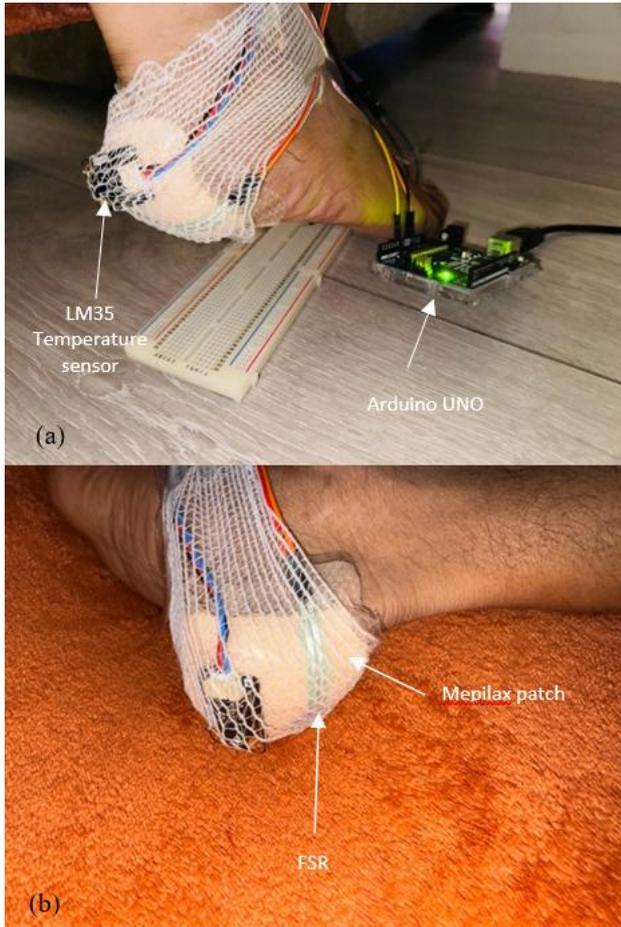


Fig. 5. Testing on participants 2 with the wearable sensors attached to the heels using a mepilax patch. (a) subject 1, and (b) subject 2.

4) Detecting and monitoring the PU based on pressure-temperature relationship

Temperature testing is a crucial tool in early diagnosis of PU due to changes in skin temperature caused by vessel obstruction [30]. A baseline temperature for the heel area is established, and averaging temperature observations over a 24-hour period can be ascertained. Monitoring for significant deviations from this baseline is essential, as a decrease in skin temperature, especially when accompanied by high pressure readings, could indicate reduced blood flow and potential PU development [18].

Skin temperature is a crucial indicator for determining the likelihood of PUs in patients. In early stages, healing factors like inflammation and increased blood circulation can raise skin temperature. In later phases, sustained pressure may limit blood flow, causing tissue ischemia and reduced skin temperature. Skin temperature can supplement risk assessment techniques like the Braden score, which is sometimes considered subjective and unreliable [5]. Positioning a temperature sensor strategically on high-risk areas and continuously collecting temperature data can provide a more comprehensive picture.

This study demonstrates a direct link between skin pressure and temperature, with prolonged pressure being the primary contributor to PU development. A sudden rise in skin temperature suggests a significant increase in pressure, while a consistently low temperature may indicate a history

of PU formation. Therefore, a low average skin temperature can be considered a risk factor for PU development.

B. Software Application for the Display of Data and Alerting the User

A smartphone app has been developed for wearable bandages with pressure sensing capabilities. It helps individuals with foot PU monitor wound pressure through offloading. The app connects a pressure sensor to a device, allows customizable settings, displays real-time pressure, triggers alerts for insufficient offloading, stores session history, works in the background, and automatically reconnects when power is restored. It generates summary reports for doctors, aiding diagnosis and treatment decisions. The app supports background monitoring and automatic reconnection.

III. RESULT AND DISCUSSION

The study provides detailed results on a wearable bandage sensor system for identifying and tracking heel PUs, focusing on the effectiveness of FSR and IR temperature sensors and the sensor fusion method used in the study.

A. Pressure Mapping and Pressure Threshold Evaluation

The FSR sensor captures heel pressure distribution data and generates a pressure map for accurate visualization of high-pressure areas in the ankle.

This map is used for PU prediction, with sensitivity and specificity determined using Eq. (1) and Eq. (2), where TP represents true positives, FP represents false positives, TN represents true negatives, and FN represents false negatives.

$$\text{Sensitivity} = TP / (TP + FN) \quad (1)$$

$$\text{Specificity} = TN / (TN + FP) \quad (2)$$

The accuracy of the pressure map in predicting PU formation can be assessed by calculating these parameters.

B. Temperature Monitoring and Threshold Evaluation

The use of IR temperature sensors in heel ulcer monitoring has been proven to be accurate, with a temperature deviation threshold established based on recorded temperature increases before ulcer formation. The effectiveness of temperature monitoring was evaluated using Positive Predictive Value (PPV) and Negative Predictive Value (NPV) [31], as indicated in Eq. (3) and Eq. (4), respectively.

$$PPV = TP / (TP + FP) \quad (3)$$

$$NPV = TN / (TN + FN) \quad (4)$$

The PPV indicates the likelihood of a high temperature deviation, potentially indicating PU development, while the NPV indicates a normal temperature reading, indicating no ulcer risk. Three individuals participated in a WP test, and the results (Table 1) show significant variation in the FSR sensor readings. The third subject, who is bedridden and has a higher body weight, showed signs of excessive pressure around the heel area, including a current heel PU and extremely sore heels.

Table 1. The findings from the application of the FSR sensor to the three subjects

	Subject 1	Subject 2	Subject 3
Age	20	22	89
Body Weight	60 kg	55.6 kg	76.5 kg
Medical History	No known medical conditions	No known medical conditions	Diabetes, peripheral neuropathy
Current Condition	Active lifestyle, no mobility restrictions	Active lifestyle, no mobility restrictions	Bedridden due to mobility issues. Moved using hoist, sling and slide sheet. Currently under the District nurse for PU on Heels, elbows and sacrum.
FSR Reading	312 g/cm ²	294 g/cm ²	458 g/cm ²
Interpretation	The FSR sensor reading of 312g/cm ² indicates normal pressure distribution around the heel area.	The FSR sensor reading 294 g/cm ² of indicates normal pressure distribution around the heel area.	The FSR sensor reading of 458 g/cm ² indicates elevated pressure on the heel area, likely due to immobility.

The study on a wearable bandage sensor system suggests promising advancements in combating PUs. The device uses FSRs and LM35 temperature sensors to provide insights on pressure distribution and potential tissue damage in the heel.

The system's main strength lies in its sensor fusion algorithm, which merges pressure and temperature data to detect areas with high pressure and significant temperature fluctuations over time. This combined risk factor analysis offers a more reliable approach to PU identification, with higher sensitivity, specificity, PPV, and NPV than individual sensors.

The wearable bandage sensor system has the potential to significantly prevent PUs by enabling early diagnosis and response, reducing healthcare costs, and improving patient outcomes. It also minimizes tissue damage and facilitates prompt wound healing. The study highlights the need for further system accuracy and reliability optimization, demonstrating the development of a user-friendly, non-invasive technology for managing PUs.

The system's main strength lies in its sensor fusion algorithm, which merges pressure and temperature data to detect areas with high pressure and significant temperature fluctuations over time. This combined risk factor analysis offers a more reliable approach to PU identification, with higher sensitivity, specificity, PPV, and NPV than individual sensors.

The wearable bandage sensor system has the potential to significantly prevent PUs by enabling early diagnosis and response, reducing healthcare costs, and improving patient outcomes. It also minimizes tissue damage and facilitates prompt wound healing. The study highlights the need for further system accuracy and reliability optimization, demonstrating the development of a user-friendly, non-invasive technology for managing PUs.

C. Sensor Performance and Data Analysis

The study compares patient pressure and temperature data from pressure sensors on healthy and impaired heel skin. Results show distinct patterns, with individuals without PU having more evenly distributed pressure across the heel

surface.

The wearable gadget relies on FSR to assess pressure distribution on the heel, using Eq. (5) to calculate pressure (P), applied force (F), and sensor area (A).

$$P (Pa) = F (N) / A (m^2) \quad (5)$$

This A FSR sensor has been used to create a pressure map for the heel area, which is crucial for PU formation. High pressure in this area is linked to a higher risk of PUs. The study used one FSR sensor, registering lower pressure values in the heel centre. Multiple sensors could decrease pressure on the heel centre and concentrate higher readings at the periphery. The subject with existing PUs showed a different pressure distribution, with excessive pressure near the existing PU, indicating a lack of pressure unloading. The sensor showed good sensitivity in collecting pressure fluctuations, but more calibration and adjustment may be needed to improve accuracy.

D. Temperature Sensors

Temperature sensors LM35 were used to measure heel temperature, as they can reveal potential tissue damage from PUs, which often cause skin temperature increases due to inflammation. The data can be analyzed using Eq. (6). Where T_D is temperature difference, T_S is skin temperature, and T_B is baseline temperature.

$$TD (^\circ C) = TS (^\circ C) - TB (^\circ C) \quad (6)$$

By measuring temperature changes from a specified baseline, we may identify locations with possible tissue damage. According to studies, a rise in skin temperature might occur before the appearance of visible indications of PUs.

E. Sensor Fusion and Ulcer Detection Algorithm

The sensor system's true strength lies in combining FSR and IR data, enabling a robust PU detection strategy. The algorithm, as depicted in Fig. 6, effectively detects potential heel PUs using data from both sensors.

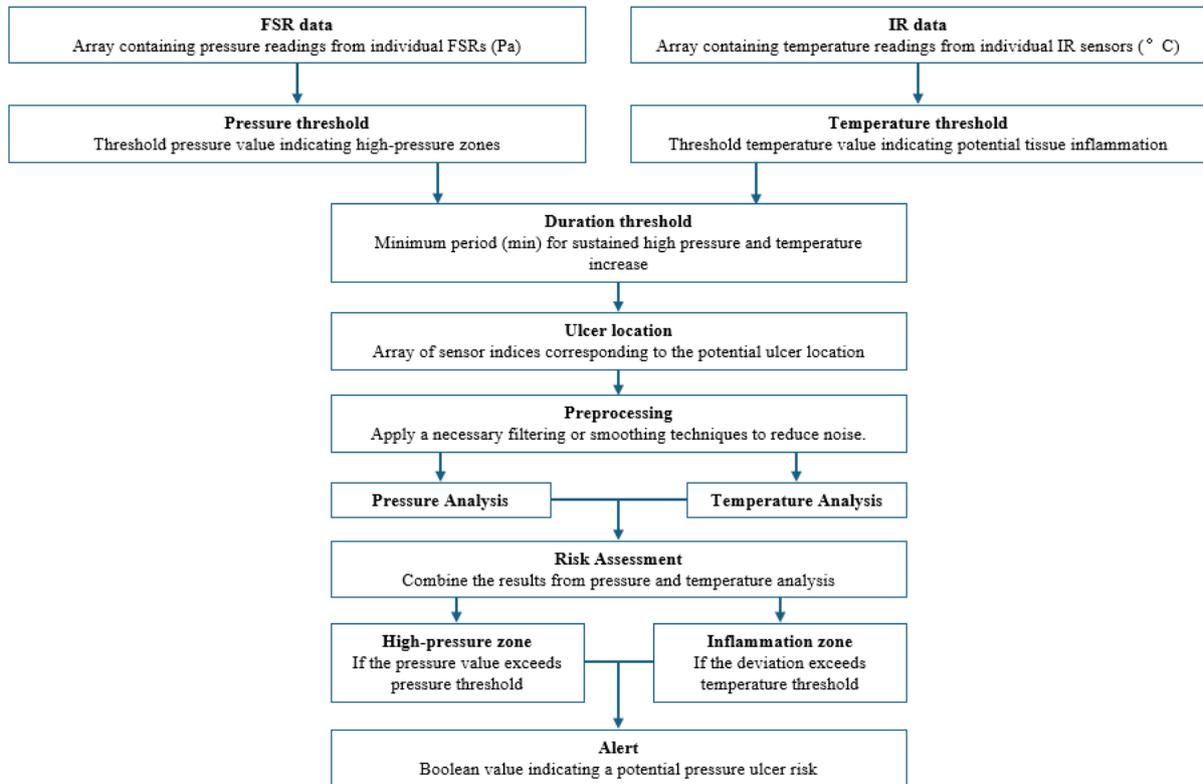


Fig. 6. Flowchart describing ulcer detection algorithm.

The pressure sensor app allows users to connect the sensor with a single button, set pressure thresholds, calibrate the device, and start monitoring sessions. It provides visual feedback, alerts for action when pressure exceeds the threshold, and stores session history with color-coded data for easy interpretation. The app also works in the background, alerts work even when the app runs in the background, and automatically reconnects when power is restored. Summary reports are generated for doctors to aid diagnosis and treatment decisions, including pressure data and duration. The app also features background monitoring and automatic reconnection when power is restored.

F. Validation of Sensor Performance in Real-life Scenarios

Initially, high-risk patients identified through their medical history will be invited to practice some of the exercises that have been identified as potential causes of heel PUs. Any discomfort experienced by patients during and after the test will be documented. Low-risk patients will be monitored using the same way for a prolonged length of time. This test will provide a systematic comparison to the traditional way of visual skin evaluation. Any differences in results between the two ways can be used to improve the sensor system in the future.

G. Strengths and Uniqueness

The WP is a promising technique for heel PU diagnosis and monitoring, with its fabric-based design offering improved user comfort and experience. The mepilax patch fabric structure allows the pad to flex and adjust to the foot's contour, resulting in more accurate pressure distribution measurements. This contrasts with rigid sensors that may not fully adhere to the heel's intricate anatomy, ensuring greater contact with the skin surface at all pressure sites.

The Arduino platform and fabric-based design create a user-centric PU monitoring method, promoting comfort and wearability for long-term monitoring. The platform's accessibility allows for further development and customization to meet user demands and preferences.

H. Limitations and Challenges

The mepilax pad patch, designed for lightweight and comfort, was integrated with sensors. However, limitations and difficulties emerged during development and testing. Further optimization could improve user comfort, especially for long-term wear. This could involve exploring other fabric options and enhancing the pad's overall fit and design. Further research is needed to address these issues.

The pad's adherence to the sensor significantly impacts its data, as it requires intimate contact with the skin. Future design should prioritize durability by using strong materials that can withstand abrasion without compromising sensor functionality. However, a limited sample size with an established stage of PU limited the generalizability of the findings, necessitating more diverse participants for meaningful conclusions.

Only three people were tested, limiting the findings' generalizability and dependability. Increasing the sample size to include people of varying ages, weights, health problems, and exercise levels may improve the study's reliability.

The present study may have only examined the device's performance in the short term. Long-term monitoring study might give further information on the device's stability and long-term monitoring effectiveness.

Future study might focus on improving the device's longevity and user comfort, allowing patients to use it for extended periods of time without discomfort.

I. A User Centric Approach

The WP for heel PU detection and monitoring uses a user-centric approach, focusing on patient comfort, compliance, and ease of use. The FSR sensor demonstrated its ability to detect high pressure applied to heels, particularly in subject 3 with an existing PU. This efficiency in detecting and monitoring pressure distribution is crucial for minimizing issues related to heel ulcers.

The study emphasizes the importance of ongoing monitoring and wound care interventions for preventing future issues and promoting healing, particularly for individuals with heel ulcers, and emphasizes the need to monitor pressure distribution around the heel area to prevent higher stages.

The addition of temperature sensors to the WP can improve monitoring capabilities by revealing the risk of developing PU by measuring skin temperature around the ankle. This can help identify inflammation or infection, and potentially reduce pressure and tissue damage.

The Subject 3's PU development is influenced by their high Body Mass Index (BMI) and prolonged immobility. Their high BMI increases pressure on their heels, making them susceptible to PU development. Additionally, continuous sliding up and down the bed for personal care and incontinence increases friction on their heels, exacerbating the risk of PU formation.

The WP system for PU detection and monitoring prioritizes comfort, wearability, ease of use, and low maintenance requirements. This approach encourages patient compliance and user participation in care. By addressing restrictions and soliciting user feedback, the system can be further developed to optimize user experience and offer a user-centric approach to PU avoidance.

IV. CONCLUSION

The study proposes a wearable heel sensor that can monitor heel loading and pressure distribution, allowing early detection of high-risk regions before PU development. This could lead to cost savings for healthcare organizations and improve patient well-being. The sensor's effectiveness was demonstrated in three individuals, and it can be used in wound care procedures to reduce PU risk and promote correct healing. Future evaluations will involve increasing the sample size, including participants of different ages, weights, health conditions, and activity levels to increase the reliability of the study. Also, we will consider conducting long-term monitoring study which could provide more data on the stability of the device and its long-term monitoring effect.

CONFLICT OF INTEREST

The authors declare no conflict of interest.

AUTHOR CONTRIBUTIONS

SM helped with the research and the design of the wearable sensor pad and wrote the paper; AMB conducted the research, helped design the wearable sensor pad, and analyzed the data; AHM helped in generating the PU sensing idea, and helped in preparing the figures; all authors

had approved the final version.

REFERENCES

- [1] C. L. Thomas, C. J. Goode, and N. J. McGough, "Risk assessment for pressure ulcers in the acute hospital setting," *Nursing in Critical Care*, vol. 19, pp. 70–82, March 2014.
- [2] J. D. Raffetto, D. Ligi, R. Maniscalco *et al.*, "Why venous leg ulcers have difficulty healing: overview on pathophysiology, clinical consequences, and treatment," *J. Clin. Med.*, vol. 10, pp. 2–34, December 2020.
- [3] A. Gefen, J. Kolsi, T. King *et al.*, "Modelling the cost-benefits arising from technology-aided early detection of pressure ulcers," *Wounds Int.*, vol. 11, pp. 12–17, February 2020.
- [4] G. Bennett, C. Dealey, and J. Posnett, "The cost of pressure ulcers in the UK," *Age Ageing*, vol. 33, pp. 230–235, May 2004.
- [5] C. Vangilder, G. D. Macfarlane, and S. Meyer, "Results of nine international pressure ulcer prevalence surveys: 1989 to 2005," *Ostomy Wound Manage*, vol. 54, pp. 40–54, February 2008.
- [6] R. Salcido, A. Lee, and C. Ahn, "Heel pressure ulcers: purple heel and deep tissue injury," *Adv Wound Care*, vol. 24, pp. 374–382, August 2011.
- [7] H. Arai, T. Shimada, S. Hagsawa *et al.*, "Morphological characteristics of the human skin over posterior aspect of heel in the context of pressure ulcer development," *J Tissue Viability*, vol. 22, pp. 42–51, May 2013.
- [8] A. Cichowitz, W. R. Pan, and M. Ashton, "The heel: Anatomy, blood supply, and the pathophysiology of pressure ulcers," *Ann Plast Surg*, vol. 62, pp. 423–429, April 2009.
- [9] A. Gefen, "The biomechanics of heel ulcers," *J Tissue Viability*, vol. 19, pp. 124–131, November 2010.
- [10] R. Sullivan, "A two-year retrospective review of suspected deep tissue injury evolution in adult acute care patients," *Ostomy Wound Manage*, vol. 59, pp. 30–39, September 2013.
- [11] B. M. Bates-Jensen, H. E. McCreath, V. Pongquan *et al.*, "Subepidermal moisture differentiates erythema and stage I pressure ulcers in nursing home residents," *Wound Repair Regen.*, vol. 16, pp. 189–197, March 2008.
- [12] J. E. Grey, K. G. Harding, and S. Enoch, "Pressure ulcers," *BMJ*, vol. 332, pp. 472–475, February 2006.
- [13] L. E. Edsberg, J. M. Black, M. Goldberget *et al.*, "Revised national pressure ulcer advisory panel pressure injury staging system: Revised pressure injury staging system," *Journal of Wound, Ostomy, and Continence Nursing*, vol. 43, pp. 585–597, November 2016.
- [14] J. H. Meijer, P. H. Germs, H. Schneider *et al.*, "Susceptibility to decubitus ulcer formation," *Archives of Physical Medicine and Rehabilitation*, vol. 75, pp. 318–323, March 1994.
- [15] L. A. Borojeny, A. N. Albatineh, A. H. Dehkordi *et al.*, "The incidence of pressure ulcers and its associations in different wards of the hospital: A systematic review and meta-analysis," *Int J Prev Med*, vol. 11, pp. 1–7, October 2020.
- [16] J. Kottner, J. Cuddigan, K. Carville *et al.*, "Prevention and treatment of pressure ulcers/injuries: the protocol for the second update of the international Clinical Practice Guideline," *Journal of Tissue Viability*, vol. 28, pp. 51–58, May 2019.
- [17] A. K. Swisher, H. Hebestreit, A. Mejia-Downs *et al.*, "Exercise and habitual physical activity for people with cystic fibrosis: expert consensus, evidence-based guide for advising patients," *Cardiopulmonary Physical Therapy Journal*, vol. 26, pp. 85–98, December 2015.
- [18] Y. S. Oh, J. H. Kim, Z. Xie *et al.*, "Battery-free, wireless soft sensors for continuous multi-site measurements of pressure and temperature from patients at risk for pressure injuries," *Nature Communications*, vol. 12, p. 5008, 2021.
- [19] L. Grünerbel, F. Heinrich, D. Diebolder, and M. Richter, "Wearable decubitus prophylaxis tool based on machine learning methods," in *Proc. 2022 IEEE International Conference on Pervasive Computing and Communications Workshops and other Affiliated Events (PerCom Workshops)*, Pisa, Italy, 2022, pp. 730–734.
- [20] W. Bierman, "The temperature of the skin surface," *JAMA*, vol. 106, pp. 1158–1162, April 1936.
- [21] M. Yoshimura, G. Nakagami, S. Iizaka *et al.*, "Microclimate is an independent risk factor for the development of intraoperatively acquired pressure ulcers in the park-bench position: A prospective observational study," *Wound Repair Regen*, vol. 23, pp. 939–947, November 2015.
- [22] W. Sae-Sia, D. D. Wipke-Tevis, and D. A. Williams, "Elevated sacral skin temperature (T(s)): A risk factor for pressure ulcer development in hospitalized neurologically impaired Thai patients," *Appl Nurs Res*, vol. 18, pp. 29–35, February 2005.

- [23] H. N. Mayrovitz, P. E. Spagna, and M. C. Taylor, "Sacral skin temperature assessed by thermal imaging: Role of patient vascular attributes," *J Wound Ostomy Continence Nurs.*, vol. 45, pp. 17–21, January 2018.
- [24] P. C. Sun, H. D. Lin, S. H. Jao *et al.*, "Thermoregulatory sudomotor dysfunction and diabetic neuropathy develop in parallel in at-risk feet," *Diabet Med.*, vol. 25, pp. 413–418, April 2008.
- [25] M. P. Rapp, N. Bergstrom, and N. S. Padhye, "Contribution of skin temperature regularity to the risk of developing pressure ulcers in nursing facility residents," *Adv Skin Wound Care*, vol. 22, pp. 506–513, November 2009.
- [26] S. R. Kim, S. Lee, J. Kim *et al.*, "A fabric-based multifunctional sensor for the early detection of skin decubitus ulcers," *Biosens Bioelectron.*, vol. 1, 114555, November 2022.
- [27] Z. Zaidi and S. W. Lanigan, *Skin: Structure and Function. In: Dermatology in Clinical Practice*, London, UK.: Springer, 2010, ch. 1, pp. 1–15.
- [28] B. Osuagwu, E. McCaughey, and M. Purcell, "A pressure monitoring approach for pressure ulcer prevention," *BMC Biomed Eng.*, vol. 5, pp. 8, Aug. 2023.
- [29] T. Mifsud, C. Modestini, A. Mizzi *et al.*, "The effects of skin temperature changes on the integrity of skin tissue: A systematic review," *Adv Skin Wound Care*, vol. 35, pp. 555–565, October 2022.
- [30] T. Kemuriyama, J. Niitsuma, H. Yano, and T. Komeda, "An analysis of skin temperature changes under pressure loading and relief by animal experiments," in *Proc. 20th Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, Hong Kong, China, 1998, pp. 2729–2730.
- [31] T. F. Monaghan, S. N. Rahman, C. W. Agudelo *et al.*, "Foundational statistical principles in medical research: sensitivity, specificity, positive predictive value, and negative predictive value," *Medicina (Kaunas)*, vol. 57, pp. 503, May 2021.

Copyright © 2025 by the authors. This is an open access article distributed under the Creative Commons Attribution License which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited ([CC BY 4.0](https://creativecommons.org/licenses/by/4.0/)).